

HACH BIOTECTOR B3500dw TOC ANALYZER

Applications
• Drinking Water



Maximum uptime and reliability for TOC analysis in drinking water applications

The Hach BioTector B3500dw uses patented technology that only requires scheduled maintenance every 6 months and delivers 99.86% uptime ensuring total confidence in your TOC measurement.

Rock solid reliability

With patented, EPA method approved Two Stage Advanced Oxidation Technology, the self-cleaning sample reactor of B3500dw delivers maximum reliability.

Lowest cost of ownership

With its 99.86% uptime, semi-annual maintenance and reagent replenishment is all that is needed.

Secure your source water

TSAO technology analyzes organics in your source that are invisible to scanning UV technologies.

Technical Data*

Parameter	TOC (NPOC), TIC, % TOC removal (with 2 streams) and COD, BOD after correlation	Sample Inlet Temperature	0 to 60 °C (36 to 140 °F)
Measurement Method	Infrared measurement of CO ₂ after oxidation (DIN EN 1484:1997-08, ISO 8245:1999-03, EPA 415.1)	Ambient Temperature	5 to 45 °C (41 to 113 °F)
Oxidation Method	Patented Two-Stage Advanced Oxidation Process (TSAO) using Hydroxyl Radicals, Hach Company method 10261 (EPA approved for drinking water)	Humidity	5 to 85 % (non-condensing)
Range	0 to 25 mg/L C	Particle Size	Up to 100 µm
Range Selection	Automatic or manual range selection	Data Storage	Previous 9999 reaction data Previous 99 fault events
Multi-Stream	Up to 2 process streams and grab sample	Display	High contrast 40 character x 16 line backlit LCD with LED backlight
Repeatability	± 3 % of reading or ± 0.03 mg/L, whichever is greater; Lower Limit of detection LOD = 0.06 mg/L	User Interface	Microcontroller with membrane keyboard
Cycle Time	Typically 6 minutes	Power Requirements (Voltage)	120 V AC
Communication	Modbus®, Profibus DP, Ethernet <i>Modbus is a registered trademark of Gould Inc.</i>	Power Requirements (Hz)	50/60 Hz
		Service Interval	6 month service intervals
		Dimensions (H x W x D)	750 mm x 500 mm x 320 mm
		Weight	101.41 lbs. (46 kg)

*Subject to change without notice.

Principle of Operation

TIC

Acid is added to lower the pH so that inorganic carbon is sparged off as CO₂. This is measured to ensure Total Inorganic Carbon (TIC) is not carried over into the TOC.

Oxidation

BioTector's patented oxidation method (TSAO) achieves total and complete oxidation of the sample, including organic carbon to CO₂. TSAO utilizes hydroxyl radicals generated within the analyzer by combining oxygen, which passes through the ozone generator, with sodium hydroxide.


TOC

To remove CO₂ from the oxidized sample, the pH of the sample is lowered again. The CO₂ is sparged and measured by the specially developed NDIR CO₂ analyzer. The result is displayed as Total Organic Carbon (TOC).




Dimensions


Front view

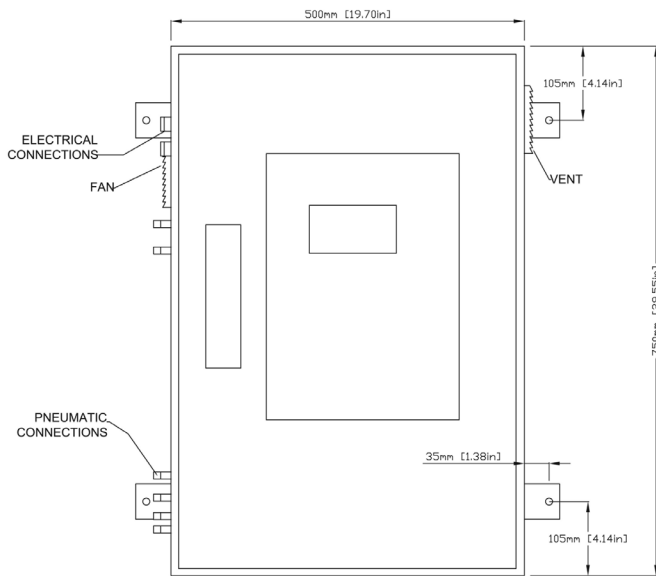


Side view

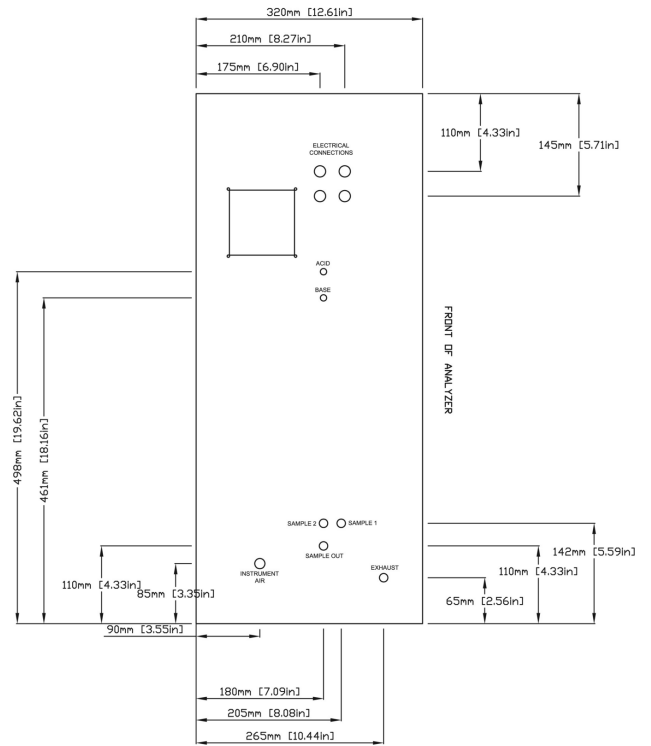

Top view

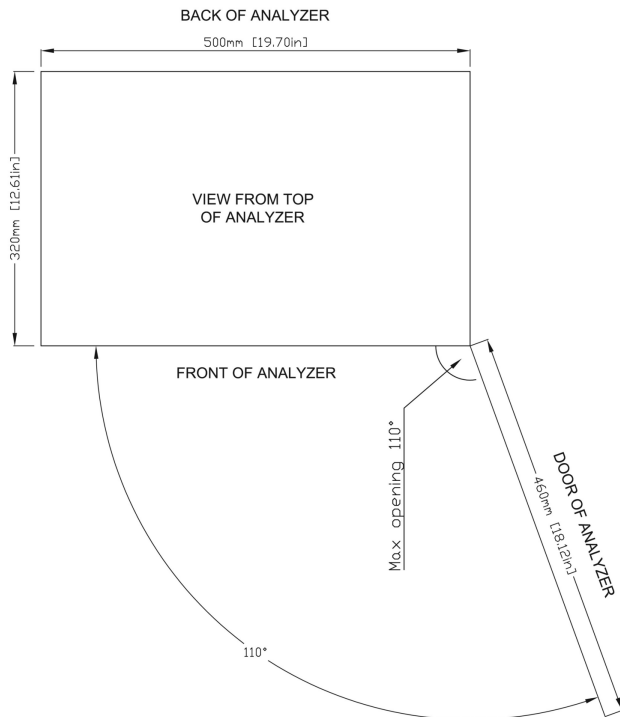

Panel detail

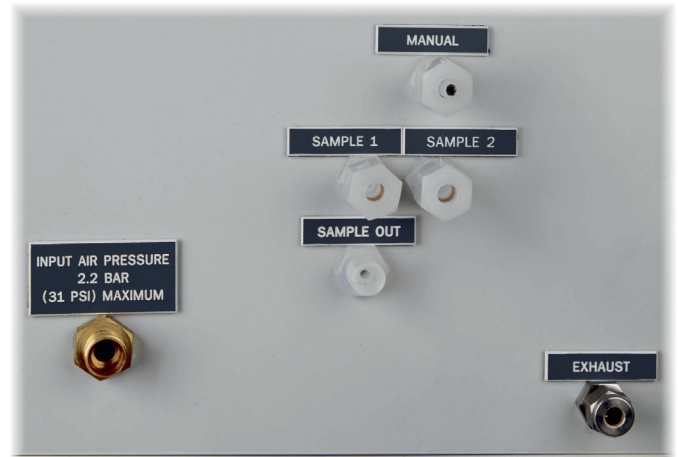

Order Information

Instruments

B0.014652000001	Hach BioTector B3500dw Online TOC analyzer, 0 - 25 ppm, 1 stream, 120 V AC
DWBCAA152AAA2	Hach BioTector B3500dw Online TOC analyzer, 0 - 25 ppm, 1 stream, 230 V AC
B0.015752000001	Hach BioTector B3500dw Online TOC analyzer, 0 - 25 ppm, 2 stream, 120 V AC
DWBCAA152AAC2	Hach BioTector B3500dw Online TOC analyzer, 0 - 25 ppm, 2 stream, 230 V AC

Accessories

19-COM-160	BioTector Compressor 115 V / 60 Hz
19-COM-250	BioTector Compressor 230 V / 50 Hz
10-SMC-001	B3500 Air supply filter pack
19-KIT-123	Six months spare part kit for BioTector B3500

Reagents

2038062	BioTector Reagent, 4.0 N NaOH
2038162	BioTector Reagent, 6.0 N Sulfuric Acid with Mn Catalysator

Be certain in your measurements with a first class Service Partner. Be confident with Hach Service.

By having regular on-site preventative maintenance and calibration, you maximise your measurement reliability and instrument uptime. Hach Service Programs give you full assurance that your instruments stay in compliance, and you stay within your budget.

Start-Up:

Commissioning will ensure you get the best performance from your instrumentation from the first day you use it.

Service Agreements:

Hach offers a wide range of service agreements that can be tailored to you to help maximise your measurement reliability and instrument uptime.

Contact us to get a service offering designed for you.

HACH World Headquarters: Loveland, Colorado USA

United States: 800-227-4224 tel 970-669-2932 fax orders@hach.com

Outside United States: 970-669-3050 tel 970-461-3939 fax int@hach.com

hach.com

Printed in U.S.A.

©Hach Company, 2016. All rights reserved.

In the interest of improving and updating its equipment, Hach Company reserves the right to alter specifications to equipment at any time.



Be Right™